

ERRATA

Erratum: "Demonstration of megavoltage and diagnostic x-ray imaging with hydrogenated amorphous silicon arrays" [Med. Phys. 19, 1455–1466 (1992)]

Larry E. Antonuk, John Boudry, Weidong Huang, Daniel L. McShan, Edward J. Morton,
and John Yorkston

Department of Radiation Oncology, University of Michigan Medical Center, Ann Arbor, Michigan 48109

Michael J. Longo

Department of Physics, University of Michigan, Ann Arbor, Michigan 48109

Robert A. Street

Xerox Palo Alto Research Center, 3333 Coyote Road, Palo Alto, California 94304

(Received 2 March 1993; accepted for publication 22 March 1993)

The images appearing in Fig. 12(a) and (b) were interchanged. The correctly labeled Fig. 12(a) and (b) along with the captions appear here.

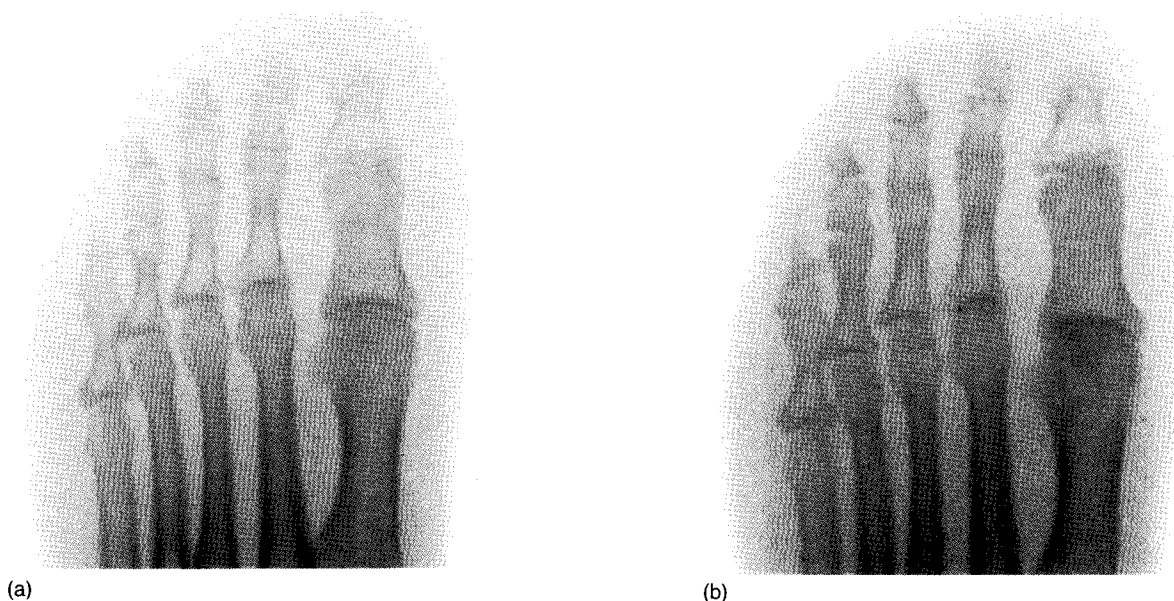


FIG. 12. Diagnostic x-ray images of a foot phantom at 65 kVp. (a) Image acquired with the 450- μ m array of Fig. 9 taken with 0.75-mAs exposure. The image processing corresponds to that of Fig. 9(c). (b) Digitized film image taken with 0.35-mAs exposure.