


Computer-Aided Design and 3-Dimensional Printing for Costal Cartilage Simulation of Airway Graft Carving

Jennifer F. Ha, MBBS¹, Robert J. Morrison, MD², Glenn E. Green, MD¹, and David A. Zopf, MD, MS^{1,3}

Otolaryngology–
 Head and Neck Surgery
 1–4
 © American Academy of
 Otolaryngology–Head and Neck
 Surgery Foundation 2017
 Reprints and permission:
sagepub.com/journalsPermissions.nav
 DOI: 10.1177/0194599817697048
<http://otojournal.org>


Sponsorships or competing interests that may be relevant to content are disclosed at the end of this article.

Abstract

Autologous cartilage grafting during open airway reconstruction is a complex skill instrumental to the success of the operation. Most trainees lack adequate opportunities to develop proficiency in this skill. We hypothesized that 3-dimensional (3D) printing and computer-aided design can be used to create a high-fidelity simulator for developing skills carving costal cartilage grafts for airway reconstruction. The rapid manufacturing and low cost of the simulator allow deployment in locations lacking expert instructors or cadaveric dissection, such as medical missions and Third World countries. In this blinded, prospective observational study, resident trainees completed a physical simulator exercise using a 3D-printed costal cartilage grafting tool. Participant assessment was performed using a Likert scale questionnaire, and airway grafts were assessed by a blinded expert surgeon. Most participants found this to be a very relevant training tool and highly rated the level of realism of the simulation tool.

Keywords

3D modeling, computer aided design, 3D printing, laryngotracheal reconstruction, surgical training, simulation, tool, anterior graft, posterior graft, costal cartilage, carving

Received October 22, 2016; revised January 27, 2017; accepted February 9, 2017.

Hands-on experience is essential for acquiring and improving surgical skills of new procedures for surgeon trainees. While these skills have historically been acquired in live patients, anaesthetized animals, or human cadavers, surgical simulation is being increasingly recognized as an important tool in surgical training.^{1–4}

Additive manufacturing, or 3-dimensional (3D) printing, has potential to augment surgical simulation in otolaryngology by facilitating production of high-fidelity models through

computer-aided design (CAD) for hands-on simulation of complex anatomy or critical procedures.^{1,4,5} When combined with thoughtful material choices, 3D printing can reproduce visuospatial and haptic characteristics of a surgical procedure.¹

Airway reconstruction performed for airway stenosis, such as laryngotracheal reconstruction, is a technically demanding procedure where costal cartilage is carved to support and expand a reconstructed trachea. Currently, a surgeon in training has scarce opportunity to carve cartilage grafts in these procedures as this highly critical portion is not amenable to suboptimal outcome. We aimed to investigate the use of 3D printing for production of a lifelike simulation tool for surgical training of carving of costal cartilage grafts for airway reconstruction.

Methods

Following University of Michigan Health System (UMHS) institutional review board exemption, simulation training was conducted during the UMHS otolaryngology–head and neck surgery dissection course.

Production of Simulation Tool

A standardized 3D-printed representation of a harvested human costal cartilage graft was created via segmentation of a computed tomography (CT) scan of a normal 8-year-old pediatric rib via previously published methods.⁶ A negative mold of the model was manufactured out of acrylonitrile butadiene styrene polymer using a fused-deposition modeling 3D printer and the simulation tool fabricated by filling the mold with a 2:1 ratio of pure cornstarch and silicone (GE Silicone II White, General Electric, Fairfield, Connecticut, USA) (**Figure 1A, B**). The

¹Division of Pediatric Otolaryngology, Department of Otolaryngology–Head & Neck Surgery, University of Michigan, Ann Arbor, Michigan, USA

²Department of Otolaryngology–Head & Neck Surgery, University of Michigan, Ann Arbor, Michigan, USA

³Department of Biomedical Engineering, College of Engineering, University of Michigan, Ann Arbor, Michigan, USA

Corresponding Author:

David A Zopf, MD, MS, Division of Pediatric Otolaryngology, Department of Otolaryngology–Head & Neck Surgery, University of Michigan, 1540 E. Hospital Drive, SPC 4-241, Ann Arbor, MI 48109, USA.
 Email: davidzopf@med.umich.edu

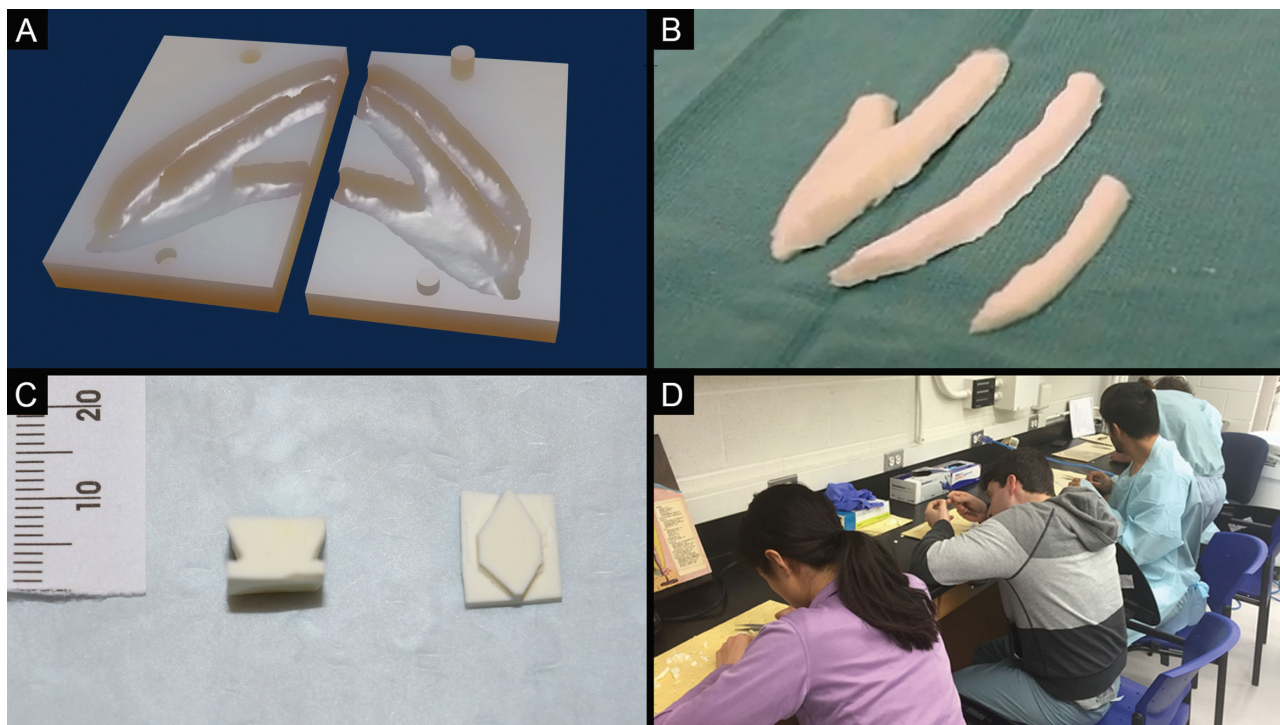


Figure 1. Three-dimensional (3D)-printed costal cartilage simulation for carving of airway grafts. (A) Three-dimensional rendering of stereolithography (.STL) file for the costal cartilage 3D-printed mold. (B) Final costal cartilage simulation tool. (C) Examples of final carved posterior (left) and anterior (right) airway grafts. (D) Trainee participants performing the simulation exercise.

composition of the material has been previously validated by microtia surgeons.⁶

Recruitment and Randomization

All otolaryngology resident trainees, including interns and rotating medical students, were invited to participate. Participants were divided per postgraduate year (PGY) and randomized by PGY level into 2 groups: (1) presimulation instructions provided by a single live demonstration by the senior author or (2) single viewing of short instructional video (Videos S1-S2, available at otojournal.org). Participants completed the simulator in groups of 5 that were heterogeneous by PGY level and instructional method.

Simulation and Assessment

All participants completed 2 sequential simulations of carving an anterior and posterior graft for airway reconstruction (**Figure 1C, D**). After completion, all participants completed a previously validated 10-item Likert scale survey that had been modified to query about the simulator characteristics (Supplemental Figure S1A, available in the online version of the article).⁷

The final graft carvings were evaluated using a Likert scale assessing accuracy and appropriateness for clinical use by a blinded expert airway reconstructive surgeon (Supplemental Figure S1B, available in the online version of the article.).

Data Analysis

Data were analyzed with SPSS Statistics (SPSS, Inc, an IBM Company, Chicago, Illinois) software. An independent

sample Student *t* test compared the mean between groups. A paired sample Student *t* test was used to compare the means of the variables. Analysis of variance (ANOVA) was used to compare the training level to factors related to the carvings. We defined statistical significance as 5% ($\alpha = .05$).

Results

There were 18 participants (4 medical students and 2 PGY-1, 3 PGY-2, 4 PGY-3, 2 PGY-4, and 3 PGY-5 trainees), with 9 participants randomized per simulation group. Of the trainees, 66.7% had not participated in an airway reconstruction procedure, with the greatest number of exposures by a participant being 6 operations. Observation of or experience in graft carving prior to the training session did not affect speed or quality of carving ($P > .05$).

In total, 78% of the participants rated this as a very relevant training tool. Of the residents who had experience in airway reconstruction procedures, 56% reported that the simulation was highly realistic. Of the learners who did not rate the simulator highly, concerns expressed included material heterogeneity and unfamiliarity of the tactile feel of normal pediatric costal cartilage.

Participants' self-assessments of confidence and efficiency increased with subsequent repetition of the simulation exercise (**Figure 2**). Both variables were associated with the time to carve both anterior and both posterior grafts ($P < .05$ for all analyses), but neither were significantly associated with expert assessments of either attempt of either graft type. Training level did not influence the

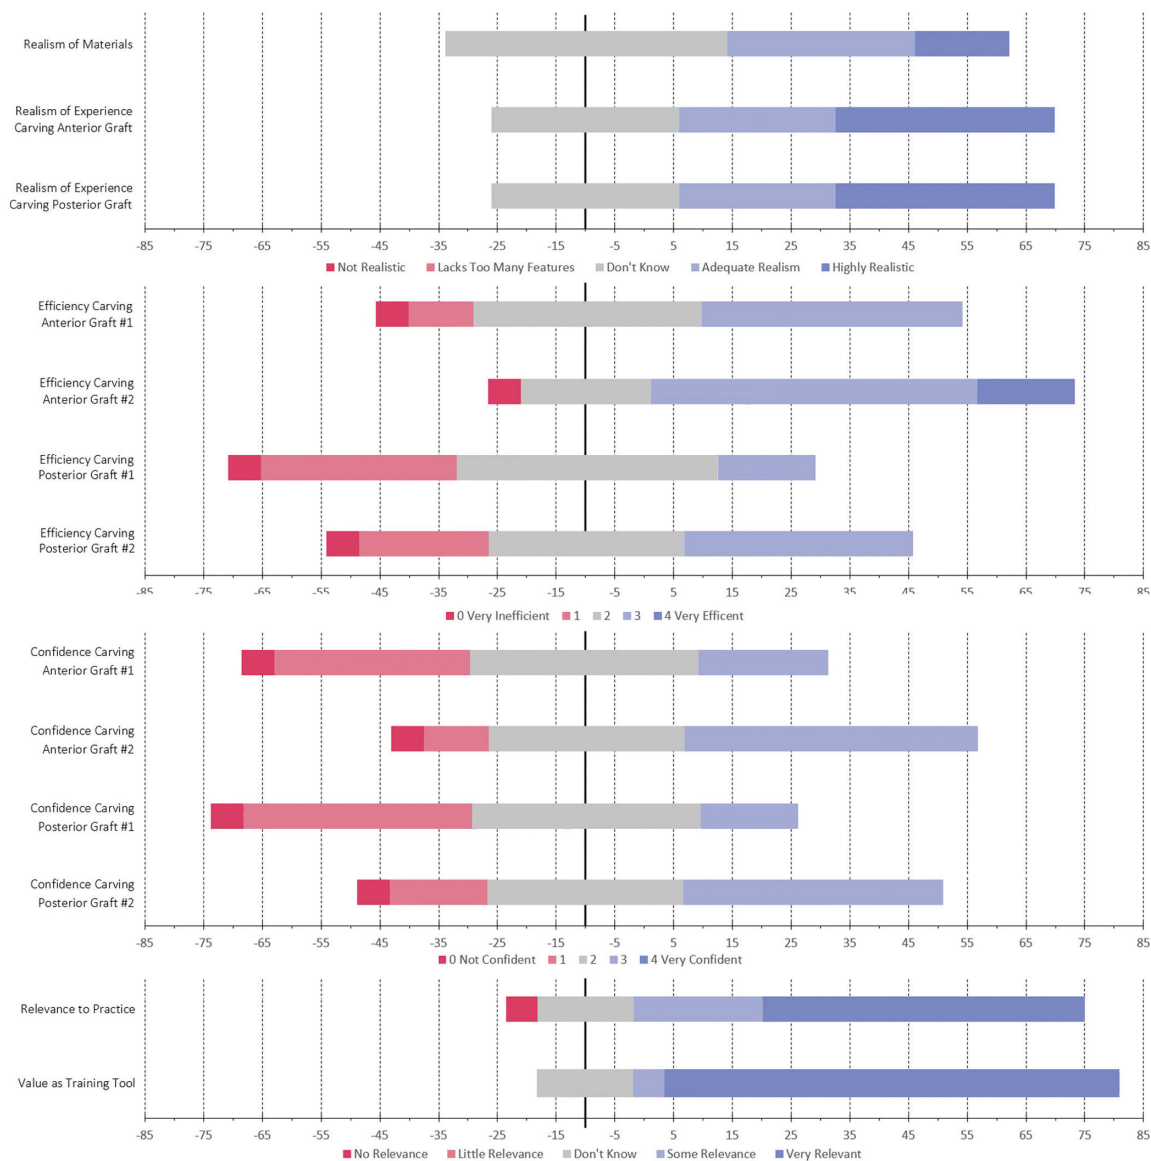


Figure 2. Participant Likert scale self-assessment results.

time it took to carve the grafts. There was no difference in the expert rating between the video demonstration and live demonstration groups for either graft type.

Discussion

Surgical simulation has previously been demonstrated to be effective for acquisition of certain surgical skills in trainees.^{8,9} We hypothesized that simulating carving of cartilage grafts for airway reconstruction may assist with skill attainment. Of importance, whereas 11% of residents had prior exposure with carving airway reconstruction grafts before the teaching session, within an hour, all participants received the experience of carving 4 grafts themselves. It is of interest to consider how that may affect future exposures and engagement in the actual operative setting.

Our results demonstrate that the simulation was rated highly by participants, who felt it was relevant and of value

to their practice as residents. Despite this, several participants commented that the material was inconsistent at times, noting that some constructs were softer and fractured more easily. We are currently refining the formula, although we suspect curing time to be essential.

No differentiation could be made between participants of different PGY levels or by number of attempts. This may be due to the heterogeneity of the participant groups, difficulty of the simulation task, lack of prior exposure by participants, and limited corrective instruction provided during or between attempts. Increased number of attempts in the simulation may be necessary before baseline performance expectations or gains in skill can be quantified.^{2,10} No differentiation could be made between educational modality (video vs live demonstration), which may be attributed to inadequate exposures to the instructional materials and limitations of the educational environment.

The material cost per simulation model was \$ 0.60, and the mold for the model was manufactured using a consumer 3D printer costing approximately \$1000. As such, this simulator is low cost and rapidly deployable in a variety of situations, including where training resources are limited. The simulator can also be customized based on individual patient imaging, allowing for patient-specific and scenario-specific simulation.

Our pilot study is limited by small sample size, which may restrict the ability to generalize findings across a broader population of otolaryngology trainees. In addition, while competency carving grafts is an important skill for airway reconstruction, it does not convey competency to perform the entire operation. The use of Likert questionnaires introduces potential for acquiescence bias, which may overrate the favorability of the simulator. Further investigation, including increased repetitions through the simulator, is necessary to assess the true effect of the simulator on surgical skill in carving airway grafts.

This pilot study demonstrates the use of CAD and 3D printing to create a rapidly producible and deployable, low-cost physical simulator for cartilage graft carving in airway reconstruction. The cost and ability for this simulation training to be done in any setting are particularly advantageous. When considering international or remote surgical training, leveraging low-cost, standardized tools such as this simulator may be an effective use of resources to assist in training surgeons worldwide.

Acknowledgments

We thank the Rontal family for their support of resident training and funding of the head and neck dissection course and Dr Deborah Rooney in the University of Michigan Clinical Simulation Center for providing the initial simulation assessment forms.

Author Contributions

Jennifer F. Ha, conceptualized and designed the project, carried out the project methods and initial data analysis, drafted the initial manuscript, and approved the final manuscript as submitted; **Robert J. Morrison**, carried out the project methods, performed data analysis, reviewed and revised the manuscript, and approved the final manuscript as submitted; **Glenn E. Green**, carried out the project methods, reviewed and revised the manuscript, and approved the final manuscript as submitted; **David A. Zopf**, conceptualized and designed the project, carried out the project methods, drafted the initial manuscript, performed data analysis, and approved the final manuscript as submitted.

Disclosures

Competing interests: David A. Zopf has filed a US patent application for the simulation device discussed in the manuscript. Robert J. Morrison, part of salary supported by NIH grant T32 DC005356-12, a research training grant.

Sponsorships: None.

Funding source: NIH grant T32 DC005356-12, which supported the salary of Robert J. Morrison during his dedicated research time in residency.

Supplemental Material

Additional supporting information is available in the online version of the article.

References

- Rose AS, Kimbell JS, Webster CE, Harrysson OL, Formeister EJ, Buchman CA. Multi-material 3D models for temporal bone surgical simulation. *Ann Otol Rhinol Laryngol*. 2015; 124:528-536.
- Wijewickrema S, Piromchai P, Zhou Y, et al. Developing effective automated feedback for temporal bone surgery simulation. *Otolaryngol Head Neck Surg*. 2015;152:1082-1088.
- Ventola CL. Medical applications for 3D printing: current and projected uses. *PT*. 2014;30:704-711.
- Scawn RL, Foster A, Lee BW, Kikkawa DO, Korn BS. Customised 3D printing: an innovative training tool for the next generation of orbital surgeons. *Orbit*. 2015;34:216-219.
- AlAli AB, Griffen MF, Butler PE. Three-dimensional printing surgical applications. *Eplasty*. 2015;15:e37.
- Berens AM, Newman S, Bhrany AD, Murakami C, Sie KC, Zopf DA. Computer-aided design and 3D printing to produce a costal cartilage model for simulation of auricular reconstruction. *Otolaryngol Head Neck Surg*. 2016;155:356-359.
- Barsness KA, Rooney DM, Davis LM. Collaboration in simulation: the development and initial validation of a novel thoracoscopic neonatal simulator. *J Pediatr Surg*. 2013;48:1232-1238.
- Costello JP, Olivieri LJ, Su L, et al. Incorporating three-dimensional printing into a simulation-based congenital heart disease and critical care training curriculum for resident physicians. *Congenit Heart Dis*. 2015;10:185-190.
- Cook DA, Hatala R, Brydges R, et al. Technology-enhanced simulation for health professions education: a systematic review and meta-analysis. *JAMA*. 2011;306:978-988.
- Firmin F, Marchac A. A novel algorithm for autologous ear reconstruction. *Semin Plast Surg*. 2011;25:257-264.